

Admn/Prop/04/2017-AIIMS.JDH

Dated: - 08th May, 2017.

Subject: Purchase of Portable Exhaled Nitric Oxide Monitor along with Sepsis Estimation System

for the department of Pediatrics at AIIMS, Jodhpur on proprietary basis - **Inviting comments**

thereon.

The Institute is in the purchase of Portable Exhaled Nitric Oxide Monitor along with Sepsis

Estimation System for the department of Pediatrics at AIIMS, Jodhpur from M/s Aerocrine, Sweden

on proprietary basis. The proposal submitted by M/s Kopran Laboratories Ltd, Mumbai and PAC

certification by user are attached.

The above document are being uploaded for open information to submit subjection,

comments, if any from any manufacturer regarding proprietary nature of the equipment within

21days of issue giving reference Admn/Prop/04/2017-AIIMS.JDH. The comments should be

received by office of Administrative Officer, Medical College at AIIMS, Jodhpur on or before 30th

May 2017 upto 03:00 PM failing which it will be presumed that any other vendor is having no


comment to offer and case will be decided on merits.

Yours faithfully,


Administrative Officer

Enclosed: Related documents enclosed.



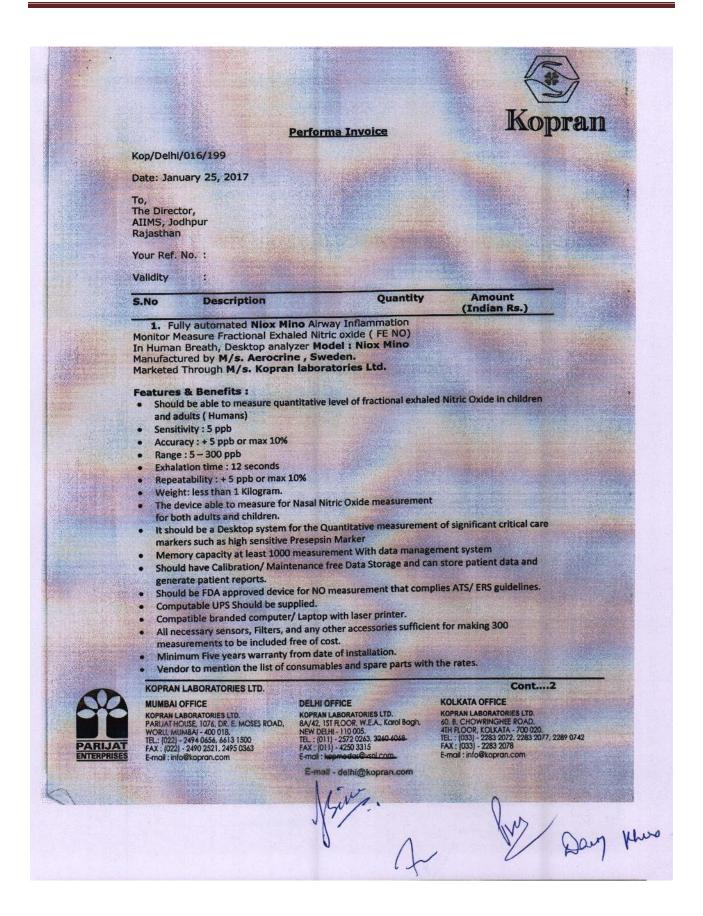



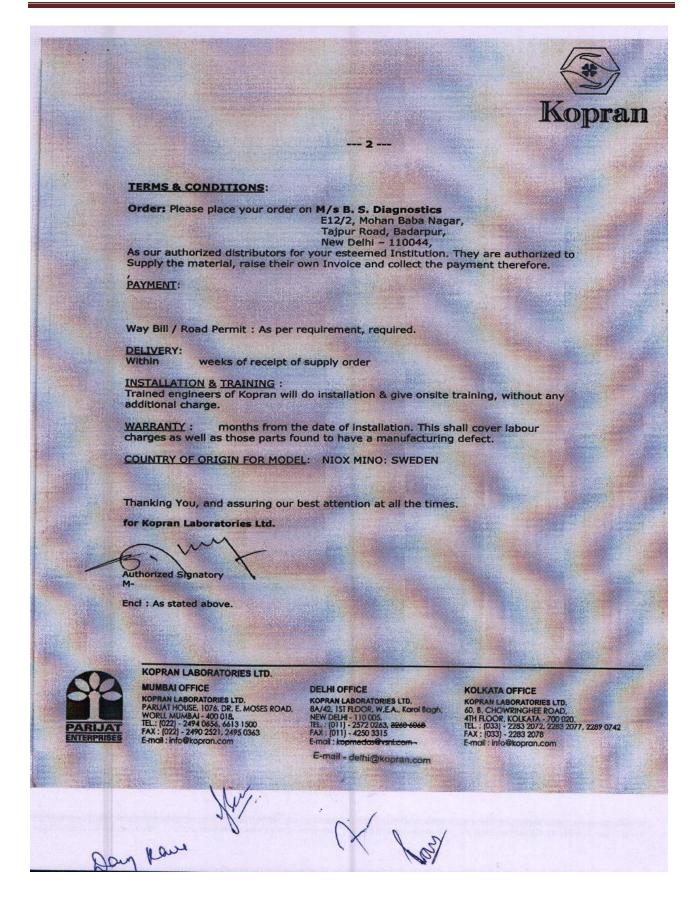







S. No.	Specification
3. NO.	Should be able to measure quantitative level of fractional exhaled Nitric Oxide
	in children and adults (Humans)
2	Sensitivity: 5 ppb
3	Accuracy: + 5 ppb or max 10%
4	Range: 5 – 300 ppb
5	Exhalation time: 12 seconds
6	Repeatability: + 5 ppb or max 10%
7	Weight: less than 1 Kilogram.
8	The device able to measure for Nasal Nitric Oxide measurement
	for both adults and children.
9	It should be a Desktop system for the Quantitative measurement of significant critical care markers such as high sensitive Presepsin Marker
10	Memory capacity at least 1000 measurement With data management system
11	Should have Calibration/ Maintenance free Data Storage and can store patient data and generate patient reports.
12	Should be FDA approved device for NO measurement that complies ATS/ ERS guidelines.
13	Computable UPS Should be Supplied.
14	Compatible branded computer/ Laptop with laser printer.
15	All necessary sensors, Filters, and any other accessories sufficient for making 300 measurements to be included free of cost.
16	Minimum Five years warranty from date of installation.
17	Vendor to mention the list of consumables and spare parts with the rates.



